


TECHNICAL DATA

Fluke BP290 2400 mAh High Capacity Li-Ion Battery for Fluke 190-Series-II

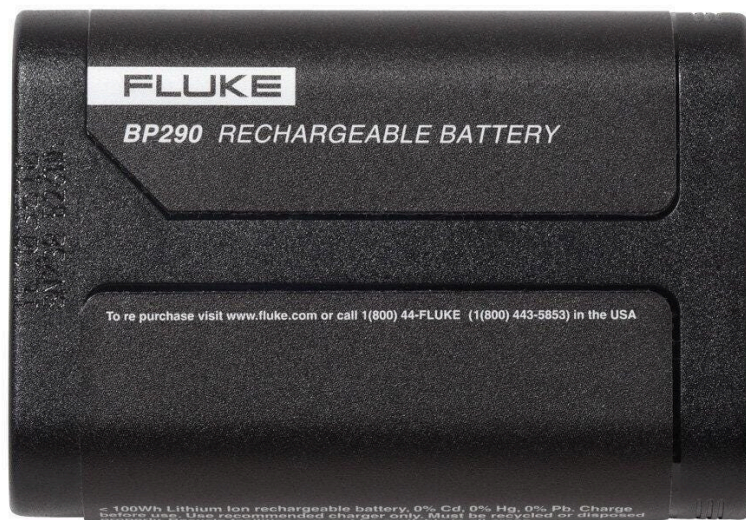

Key features

- 2400 mAh rechargeable Li-ion battery
- Compatible with ScopeMeter® 190 Series III, 190 Series II, 120B Series, MDA-500 Series Motor Drive Analyzers and 430-II Series Power Quality Analyzers

Product overview: Fluke BP290 2400 mAh High Capacity Li-Ion Battery for Fluke 190-Series-II

The Fluke BP290 Li-ion Battery is a standard capacity battery for use in Fluke 190 Series II and Series III ScopeMeter Test Tools, 120B Series ScopeMeter Test Tools, MDA-500 Series III Motor Drive Analyzers and 430-II Series Power Quality Analyzers. BP290 Li-ion batteries include a charge-status indicator so you can quickly and easily verify charge status in the field, and may be charged either in the instrument itself, or using the option [EBC290 External Charger](#). For situations requiring longer battery operating time consider the [Fluke BP291 4800 mAh High Capacity Li-Ion Battery](#).

Specifications: Fluke BP290 2400 mAh High Capacity Li-Ion Battery for Fluke 190-Series-II

Battery	Li-ion, 10.8 V, 2500 mAh, 27 Wh configuration 3ICR19/66
Safety	Pollution degree 2
Operating temperature	0 °C to +50 °C (charging may slow or stop at environmental temperatures >40 °C)
Storage temperature	-20 °C to +60 °C
Recommended storage temperature	<35 °C
Humidity	0 °C to 10 °C noncondensing 10 °C to 30 °C @ 95 % (±5 %) rh 30 °C to 40 °C @ 75 % (±5 %) rh
Altitude	3000 m
Weight	175 g
Dimensions	22 mm x 85 mm x 59 mm

Ordering information



Fluke BP290

Part#: 4025762

UPC#: 095969601849

2400 mAh High Capacity Li-Ion Battery for Fluke 190-series II

Fluke. *Keeping your world up and running.®*

Fluke Corporation
PO Box 9090, Everett, WA 98206 U.S.A.

For more information call:
In the U.S.A. (800) 443-5853
In Canada (800) 36-FLUKE
From other countries +1 (425) 446-5500
www.fluke.com

©2026 Fluke Corporation.
Specifications subject to change without notice.
08/2026

**Modification of this document is not permitted
without written permission from Fluke
Corporation.**